

Highspeed

Maintenance Procedure After Every Patient


1 Clean & Dry

- **KEEP HEAD OF THE HANDPIECE UP IN VERTICAL POSITION.**

Scrub handpiece with soft brush and warm water to remove debris.

- **OBSERVE ALL CAUTIONS LISTED!**

Towel dry handpiece thoroughly.

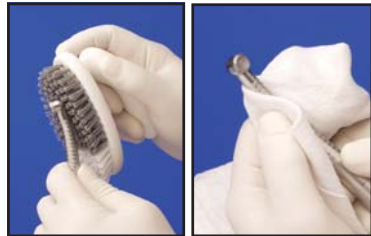

2 Lubricate and Operate

Using a **well-shaken** can of Lares Handpiece Conditioner with lube nozzle, attach handpiece and apply conditioner for **TWO SECONDS** over a towel or sink. With bur in place, run handpiece at full speed **without water** for **45 SECONDS** to expel excess conditioner.

Dry exterior of handpiece with a towel.



3 Insert into Bag and Cycle

Remove bur, bag handpieces individually and autoclave or chemiclave per manufacturer's instructions.

- **DO NOT** exceed 275 °F (135 °C).

Remove from autoclave immediately after cycle and allow to cool.

CAUTION: HANDPIECE MAY BE TOO HOT TO HANDLE!



4 Clean Fiber Optics

When handpiece is cool to the touch, gently clean fiber optic light transmitting surfaces on both ends of handpiece with cotton swab dampened with isopropyl alcohol.



Maintenance of the Swivel Model Only

Once each week inspect external surface of male swivel connection for cracked or nicked o-rings and wear. Verify that light bulb sleeve is secure.

REMINDER: FLUSH HOSE COMPLETELY OF ANY CLEANER.



IMPORTANT:

This supplement is intended as a convenient reminder of limited product information only. For complete product and maintenance information, see instruction booklet.

Lowspeed

Maintenance Procedure After Every Patient

1 Remove Attachments

Remove attachment from air motor. Remove heads from contra angle/straight attachments. Remove all burs, prophylaxis, etc. from heads and straight attachments.



2 Clean and Dry

Scrub handpiece with soft brush and warm water to remove debris.

- **OBSERVE ALL CAUTIONS LISTED!**

Towel dry equipment thoroughly.



3 Lubricate Heads Only

Apply Lares Handpiece Conditioner to all lowspeed heads. Follow specific instructions detailed in instruction booklet. It is not necessary to lube air motor, straight attachment or contra angles.



4 Insert into Bag and Cycle

Insert all components into autoclave bag and load into autoclave/chemiclave.

- **DO NOT** exceed 275 °F (135 °C). Remove immediately after cycling and allow to cool.

IT IS NOT NECESSARY TO LUBE AFTER CYCLING.

