


Engler Engineering Corporation

Instructions for replacing a connector (knuckle) on the Dynax Gurney / Dynax EZ-Glider

Using the gurney diagram, circle the connector(s) that you would like to replace.

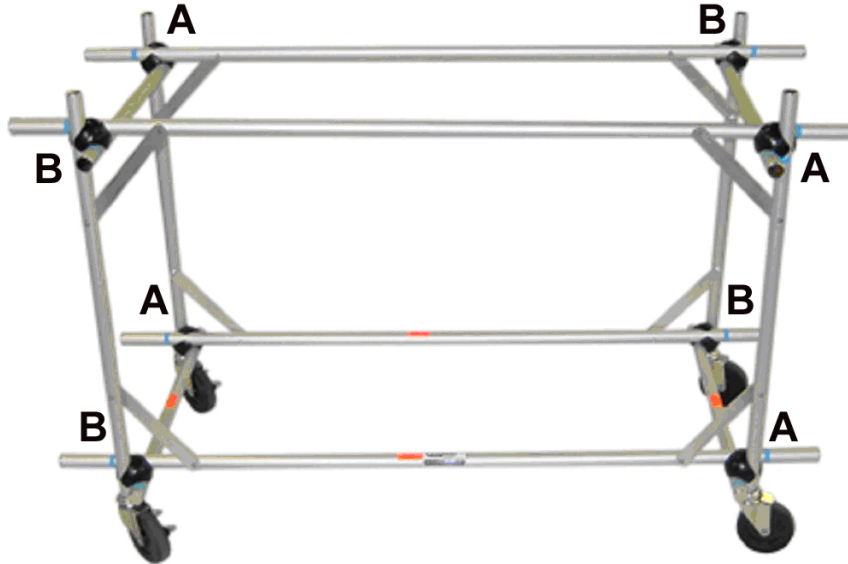

When you assemble the new connector on your **Dynax Gurney / EZ-Glider**, take care not to over tighten the screw, just snug it firmly. The gurney's metal braces do all the "heavy lifting", the connectors provide a "supporting role". If the connector is needed on the bottom of the gurney, it should rest on the caster, no need to over tighten, just snug will do.

Please note: The color of the connectors may vary.

What we need from you,

Contact / Clinic Name _____

Clinic Phone _____

Clinic Address _____

Quantity of connectors _____

Credit Card _____ Exp. ____/____/____ CCV _____

Fax your request back to us at 305-681-1620



Web: www.englerusa.com / Email: info@englerusa.com
www.dynaxusa.com / www.ez-stretcher.com / www.ez-dentaltable.com /
www.25KSeries.com for brochures, manuals and "how to"
pages please visit www.engler411.com



Proudly made
in the U.S.A.

Engler Engineering Corporation
1099 East 47th Street - Hialeah, Florida 33013 USA
Tel: (800) 445-8581 / (305) 688-8581 / Fax: (305) 685-7671